


Incontinence Sensor Pad

Steps to Install the Incontinence Sensor

1. Check the sensor for any visible defects or damage. If damage is visible the sensor pad should be replaced.
2. Verify that the pad is attached to the correct port on the white control box (shown below).

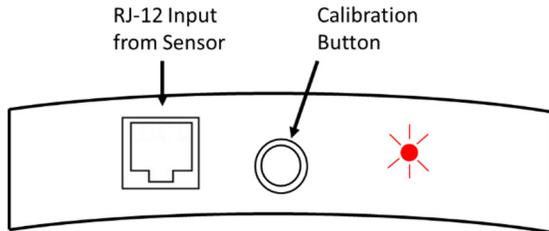

Locate the Incontinence Sensor Mat underneath the bed clothes with the pattern facing up. Position the Sensor Mat across the bed in an appropriate position, with the connector disks located at the edge of the mattress where the cable is to exit. It is important that an absorbent material of some sort be located above the Sensor Mat. This absorbent material may be a bed sheet, a towel, or a mattress pad.

3. The Sensor Mat should be oriented such that the cable and control box are positioned opposite the bed side where the patient typically gets in and out of bed.
4. If the non-absorbent nature of the Sensor Mat interferes with patient comfort, we suggest placing a bath towel over the Sensor Mat.
5. If the control box is new, pull out the plastic battery tab located on the underside of the unit. The tab is not needed for use and can be discarded.
6. To test for correct operation, short the two magnetic connectors together, and verify that the alarm system operates correctly.
7. Secure the control box to the bed by either (a) adhering it to the side of the bed or (b) tucking the control box between the mattress and box spring.
8. Verify that all cables have been secured to eliminate tripping hazard.

Cleaning the Sensor Pad

1. Wipe down with moistened cloth using only soap and water, and wipe dry. Avoid using any cleaning agent containing bleach (sodium hydroxide) as an ingredient. **DO NOT MACHINE WASH!**
2. Carefully wipe down and clean the cable, checking for any damage that may have occurred.
3. **DO NOT** immerse the pad in any liquid.
4. After cleaning the sensor, repeat all of the installation steps when replacing the sensor.

Storage

1. Store the sensors flat and **DO NOT** bend or roll the sensors.
2. The sensors are intended for normal indoor use in relatively low humidity environments.

Care and Use

1. Never pull on or jerk on the cable. Doing so may damage the connector or the mat.
2. Verify that the pad is lying flat on the mattress and that it is not bent or folded over.
3. Replace the batteries every two years by removing the top cover of the white control box. The device takes (2) AAA batteries.

Note for Sensor Signal Delay Time:

The sensor may have been preprogrammed with a signal delay, typically between 3-10 seconds. Please refer to the SmartBox Part Number to determine the preset delay time.